

# Computer-assisted Surgery and Computer-assisted Telesurgery in Otorhinolaryngology

---

**Klapan, Ivica; Vranješ, Željko; Rišavi, Ranko; Šimičić, Ljubimko; Prgomet, Drago; Glušac, Branko**

*Source / Izvornik:* **Ear, Nose & Throat Journal, 2006, 85, 318 - 321**

**Journal article, Published version**

**Rad u časopisu, Objavljena verzija rada (izdavačev PDF)**

*Permanent link / Trajna poveznica:* <https://um.nsk.hr/um:nbn:hr:239:555128>

*Rights / Prava:* [Attribution-NonCommercial 4.0 International/Imenovanje-Nekomercijalno 4.0 međunarodna](#)

*Download date / Datum preuzimanja:* **2024-11-26**



*Repository / Repozitorij:*

[Repository UHC Osijek - Repository University Hospital Centre Osijek](#)

# Computer-assisted surgery and computer-assisted telesurgery in otorhinolaryngology

Ivica Klapan, MD, PhD; Željko Vranješ, MD, PhD; Ranko Rišavi,<sup>†</sup> MD, PhD; Ljubimko Šimičić, BSEE; Drago Prgomet, MD, PhD; Branko Glušac, MD

## Abstract

*Surgical preparation is enhanced by the availability of computer-generated three-dimensional models that allow surgeons to explore the surgical field in various projections prior to an actual operation. In fact, with adequate computed tomography images, an entire operation can be simulated beforehand so that surgeons can plan the safest and most effective approach and be prepared to avoid or overcome obstacles during the actual procedure. Also, computer technology allows surgeons to conduct remote consultations and to even perform telesurgery—that is, to operate on a patient from a great distance. In this article, we describe our experience with computer-assisted local and remote endoscopic sinus surgery in Croatia.*

## Introduction

In 1992, a rhinosurgical research team was organized in the Department of Otorhinolaryngology–Head and Neck Surgery at the Zagreb University School of Medicine and the Zagreb University Hospital Centre in Croatia. The members of this team developed a novel approach to head and neck surgery: three-dimensional computer-assisted functional

endoscopic sinus [micro]surgery (3D-C-FESS). On May 12, 1994, the first 3D-C-FESS in Croatia was carried out in the Department of Otorhinolaryngology–Head and Neck Surgery at the Clinical Medical Centre in Zagreb. The patient was a 12-year-old boy who had been blinded in the left eye by a gunshot wound. The bullet had damaged the left orbit, lower eyelid, and conjunctiva and caused profuse retinal, preretinal, and subretinal hemorrhage. The vitreous body was diffusely tinged with blood. The surgery was successful, and 6 years later the boy's left eye and vision were completely normal.

On May 15, 1996, a rhinosurgical research team at Zagreb University conducted the first remote radiologic surgical teleconsultation as part of the 3D-C-FESS project. The preoperative teleconsultation took place in Zagreb between physicians at Clinical Medical Centre Šalata and physicians at Merkur University Hospital.

On October 22, 1998, the rhinosurgical research team conducted the world's first remote 3D-C-FESS.<sup>1,2</sup> Since then, we have taken part in several other telesurgeries. In this article, we describe what we have learned during this experience.

## Rationale for computer-assisted surgery

Although computed tomography (CT) is a very effective aid in planning and performing endoscopic surgery in the head and neck,<sup>3,4</sup> it does have some limitations. For example, sometimes it is not possible to precisely localize the tip of an instrument in the operative field relative to the target site shown on the CT image. In such cases, surgeons must rely on their experience and perhaps even intuition to complete an operation. An alternative to CT is computer-assisted three-dimensional visualization, which offers surgeons a considerably better view of the operative field in real time (figure 1).<sup>5</sup>

## DICOM standards

The main requisite for a computer-assisted visualization system is a high-quality image. The development of systems

<sup>†</sup> Deceased.

From the Division of Plastic and Reconstructive Head and Neck Surgery and Rhinosinusology, Department of Otorhinolaryngology–Head and Neck Surgery, Zagreb University School of Medicine and Zagreb University Hospital Centre, Zagreb, Croatia (Dr. Klapan, Dr. Rišavi, and Dr. Prgomet); the Reference Centre for Computer-Aided Surgery and Telesurgery, Ministry of Health, Zagreb (Dr. Klapan, Dr. Vranješ, Dr. Rišavi, and Dr. Glušac); the Department of Otorhinolaryngology–Head and Neck Surgery, Osijek University School of Medicine and Osijek University Hospital, Osijek, Croatia (Dr. Vranješ); the Department of Physics, University of Zagreb (Dr. Šimičić); and the Division of Otorhinolaryngology, Makarska Medical Centre, Makarska, Croatia (Dr. Glušac).

Reprint requests: Professor Ivica Klapan, MD, Department of Otorhinolaryngology–Head and Neck Surgery, Zagreb University School of Medicine, Šalata 4, HR-10000 Zagreb, Croatia. Phone: 385-1-492-0038; fax: 385-1-492-0632; e-mail: telmed@mef.hr

This work was supported in part by an unrestricted grant (No. 0108543) to Dr. Klapan from the Ministry of Science, Education, and Sport, Republic of Croatia.





Figure 1. Computer-assisted visualization is a good alternative to CT.

for data exchange between multiple diagnostic instruments and computer networks led to the establishment of DICOM standards, which codify the forms and modes of data exchange. DICOM is an acronym for *Digital Imaging and Communications in Medicine*.<sup>6</sup>

Before DICOM standards became widely accepted, image recordings were stored on film. But even under ideal conditions, film could record only 16 different image levels at most. Also, the process of transferring film images onto computer storage disks resulted in the loss of some anatomic information and the probable introduction of unwanted artifact. Moreover, the level setting and window width of the images could not be changed.

Because video images seen on diagnostic device monitors are considerably better than film images, they are used for storage in computer media. These video images are capable of containing as many as 256 image levels, and it is possible to subsequently modify the level setting and window width once they have been stored in the computer system.

When images are transferred to computer systems in accordance with DICOM protocols, they are stored in the same form that was generated by the diagnostic device without data loss. This is particularly important when images are retrieved for use during complex examinations and during preoperative preparation, as a precise demarcation is needed to distinguish diseased from healthy tissue. DICOM images can be visualized from different aspects and used to develop three-dimensional models.

### Computer-assisted preoperative preparation

Surgical preparation is enhanced by the availability of three-dimensional models that allow surgeons to explore the surgical field in various projections and to simultaneously view multiple model sections (figure 2). With programs such as Virtual Endoscopy and Virtual Surgery, an entire operation can be simulated prior to the actual surgery



Figure 2. A three-dimensional model shows the cranial anatomy.



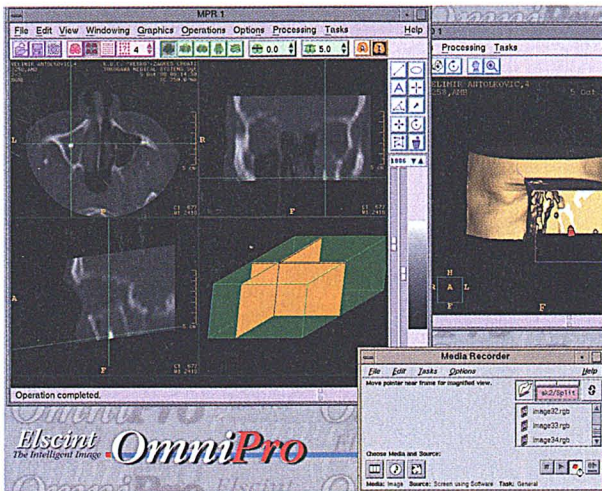


Figure 3. With programs such as Virtual Endoscopy, entire operations can be planned and simulated prior to the actual surgery.

(figure 3).<sup>7,8</sup> As a result, surgeons can plan the safest and most effective approach and be prepared to avoid or overcome obstacles during the actual procedure. Also, these models can be entered into a variety of software programs and transmitted to distant radiologic and surgical sites for preoperative consultation (Tele-Virtual Endoscopy).<sup>1,9</sup>

The development of our 3D-C-FESS system involved the use of a variety of computer programs and systems. The initial modeling was done with VolVis, VolPack/vpender, and GL Ware programs on a DECstation 3100 computer. As programs were upgraded and refined, we subsequently used 3D Viewnix V1.0 and V1.1 software, the AnalyzeAVW system, the T-Vox system, and the OmniPro 2 system on Silicon Graphics O2, Origin200, and Origin2000 computers.

### Computer-assisted surgery

The use of a computer during surgery/telesurgery requires highly reliable, stable, and fast computer systems. Computer work stations with UNIX-compatible operating systems are most commonly used. Because a surgeon's hands are engaged in performing surgery, he or she cannot operate the computer, and the presence of a computer system expert in the operating theater is necessary. However, a surgeon can operate some computer systems by voice. Model movements on the monitor and various projections and sections can be viewed by issuing simple, short voice instructions during surgery.

During our initial computer-assisted procedures, spatial orientation within the operative field of a three-dimensional computer model and transfer of a particular point to the real operative field within the patient were performed by arbitrary approximation of the known reference points of the operative field anatomy.<sup>10</sup> In this way, the given enti-

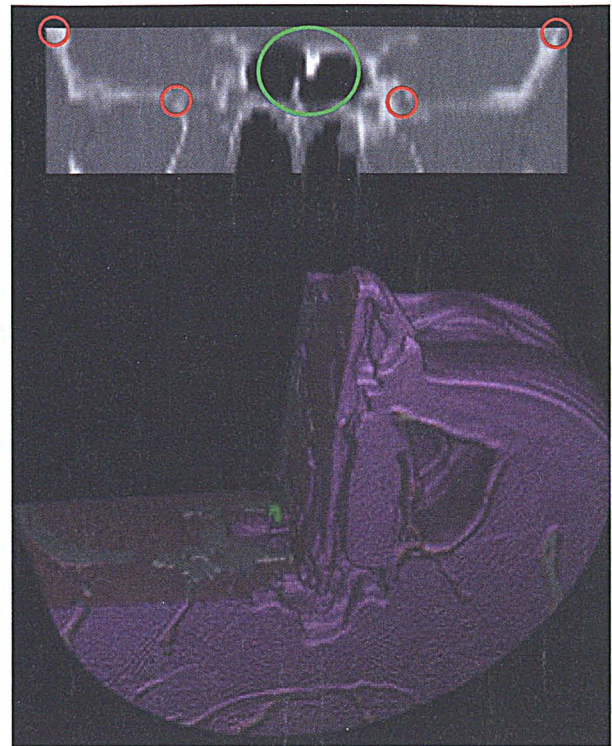


Figure 4. The major problem with computer-assisted surgery is transmission of the actual operative-field coordinate system to the coordinate system of the three-dimensional spatial model.

ties were simultaneously recognized on the model and in the real operative field.<sup>11</sup> This method facilitated access to the operative field, but it could not guarantee absolute safety at critical points.

The use of a three-dimensional spatial model of the operative field during surgery has pointed to the need for simulating the position of the tip of the instrument (e.g., endoscope and forceps) within the computer model. The major problem is transmission of the actual operative field coordinate system to the coordinate system of the three-dimensional spatial model that has been previously designed from a series of CT images during preoperative preparation (figure 4).<sup>10,12</sup>

Several modes of instrument localization within the operative field are used—electromagnetic, optic, and mechanical:

- The electromagnetic method is very sensitive to environmental electromagnetic fields (e.g., those generated by electrical devices) and to large amounts of metal (e.g., cabinets, tables, and instruments). Therefore, the basic default precision of localization within the field is inadequate for surgery.

- Optic locators have proved to be suitable, but they are relatively expensive and less precise than mechanical locators.





# NeilMed<sup>®</sup> SINUS RINSE™



*Do you routinely recommend large volume nasal saline irrigation post endoscopic sinus surgery?  
Do you differentiate between nasal saline sprays and large volume saline irrigation?  
Do you select nasal irrigation as a first line of treatment for Rhinosinusitis symptoms prior to any corticosteroids and antihistamines?*

If You said **“YES”** To Any of The Above Questions,  
**NeilMed's SINUS RINSE™** is the **#1** OTC prescribed system when it comes to **volume** irrigation of nasal and sinus passages.



**SINUS RINSE™ Kit**  
(50 PACKETS)



**SINUS RINSE™ Mixture Packets**  
(100 PACKETS)



**SINUS RINSE™ Bottle Kit**  
(5 PACKETS)

### Relieves Allergies & Sinus Symptoms

- Nasal Allergies & Dryness
- Sinus Pressure & Nasal Stuffiness
- Nasal Symptoms from Flu & Cold
- Nasal Irritation from Occupational Dust, Fumes, Animal Dander, Grass, Pollen, Smoke, & House Dust
- Post Nasal Drip & Nasal Congestion

### Advantages


- Soothing, No Burning or Stinging
- Preservative, Iodine & Latex Free
- Premixed Packets of USP Grade Sodium Chloride & Sodium Bicarbonate (Natural Ingredients & 99.9% Pure)
- pH Balanced & Isotonic Solution
- Natural relief from allergies & sinus symptoms
- Custom Designed Cap to fit any nasal opening
- Smooth Flow with easy-squeeze bottle
- Empties 100% in upright position
- Great to use after sinus surgery
- Safe during pregnancy
- Travel-size kit
- Money back guarantee\*

\*If returned within 90 days from the date of purchase



**SINUS RINSE™ Pediatric Kit**  
(50 PACKETS)

**SINUS RINSE™ Pediatric Packets**  
(100 PACKETS)



**SINUS RINSE™ Pediatric Bottle Kit**  
(5 PACKETS)

**SINUS RINSE™ Hypertonic Packets**  
(70 PACKETS)



Now Available in the USA at:

**Walgreens**

**Longs Drugs**

**KAISER PERMANENTE<sup>®</sup>**  
(OTC Pharmacy)

**Albertsons<sup>®</sup> Osco**  
(Arizona Locations Only)

**OscoDrug**

**Savon drugs**

**Jewel-Osco**

**Duane reade**

**BARTELL DRUGS**  
Washington's Own Drugstores

**ShopKo**  
STORES INC.

**meijer**  
Higher Standards. Lower Prices.

**SNYDERS**  
Drug Stores

Now Available in Canada at:

**JEAN COUTU**

**Zellers**

**Pharma Plus<sup>®</sup>**

**Herbies**  
for DRUG & FOOD

**Rexall**

**Lawtons**  
DRUGS

as well as participating IDA, Guardian, Medicine Shoppe stores.

**NeilMed<sup>®</sup>**  
PHARMACEUTICALS, INC.

Toll Free in USA & Canada 1-877-477-8633

www.neilmed.com



Patented  
Formula

# NeilMed<sup>®</sup> SINUS RINSE™

Patented  
Device

The **ONLY** Patented, USP Grade (99.9% Pure) **Sodium Chloride & Sodium Bicarbonate Mixture** available for a Moisturizing & Soothing Nasal Rinse for natural relief from allergies and sinus symptoms.

For **Volume** Therapeutic Saline Nasal Irrigation,  
Moisturization & Daily Nasal Hygiene

**NasaDOCK™**



New Extra Large  
Rinse Bottle  
16 oz. (480 mL)



Standard Regular  
Bottle  
8 oz. (240 mL)




Pediatric Bottle  
4 oz. (120 mL)



Special Use Drug  
Delivery Bottle  
2 oz. (60 mL)

New

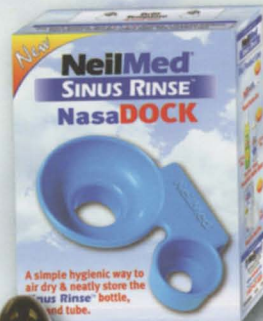

A simple  
hygienic way to  
air dry & neatly  
store the  
SINUS RINSE™  
bottle, cap  
and tube.



Hypertonic Packets



Regular Packets



Pediatric Packets

Now, Soothing  
Saline Nasal  
Rinse is as  
easy as...



1.



2.



3.



USA

1221 FARMERS LANE  
STE. 500  
SANTA ROSA, CA 95405  
TEL: (707) 525-3784  
FAX: (707) 525-3785



**NeilMed<sup>®</sup>**  
PHARMACEUTICALS, INC.

Toll Free in USA & Canada 1-877-477-8633 [www.neilmed.com](http://www.neilmed.com)  
NeilMed Pharmaceuticals Australia Pty. Ltd. Toll Free in Australia: 1800 158 900

CANADA

P.O. Box #3553  
MARKHAM, ONTARIO  
L3R 6G8

TEL: (905) 480-0202  
FAX: (905) 480-0201

**DO NOT settle for other products, as there is NO equal substitute to our Patented System.**



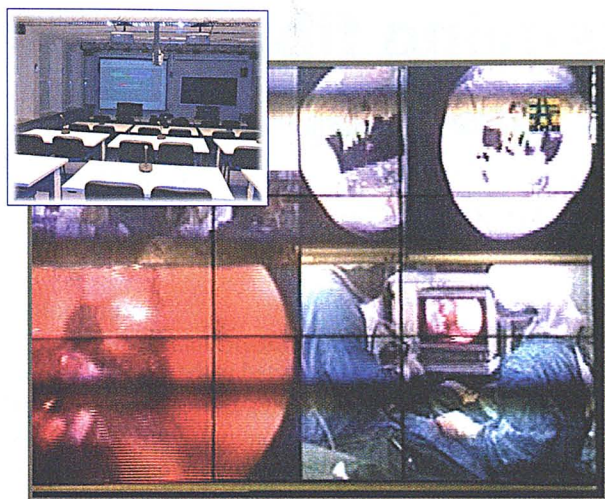


Figure 5. Computer-assisted telesurgery can be performed at a distance with the assistance of video and audio transmission and sophisticated endoscopic cameras.

- The primary shortcoming of mechanical locators is their inability to reach deep areas within the operative field. This problem might be solved by redesigning instruments so that the tips are thinner and longer.

### Teleconsultation and telesurgery

Computer-assisted consultation and surgery can be performed at a distance with the assistance of video and audio transmission and sophisticated endoscopic cameras (figure 5). Preoperatively, a consulting surgeon can receive CT images from a remote location, examine the images, develop a three-dimensional spatial model, and transfer all this information back to the remote location.<sup>2</sup> Intraoperatively, staff and consultants both near to and far from the actual operating table can view the operation "live" via the endoscopic camera images, and they can follow the progress of the surgery on the three-dimensional computer models.<sup>1,2</sup> In most cases, a network can be set up so that intraoperative consultations can be obtained from multiple locations. The underlying principle behind telesurgery is that it is often better to move the data than to move the patient.

### Postoperative analysis

All relevant pre- and intraoperative data (e.g., CT images, test results, three-dimensional models, and video of the surgery) can be stored on a CD-ROM disk and reviewed for postoperative analysis.<sup>7</sup> An analysis and critique of a computer-assisted surgical procedure may identify shortcomings and areas that need improvement. This may be especially valuable when reviewing the particularly critical points of an operation. Such a record is also useful as a teaching tool and as permanent documentation in case a medicolegal issue arises.

### Computer networks

Once a local DICOM-compliant computer-assisted surgery system is established, the next step is to create an interactive network of such programs among appropriate institutions. With such a network, physicians at participating institutions can consult almost instantaneously with each other and transmit textual, image, and other data. Of course, the consultation itself can be recorded and stored for further use.

### Acknowledgment

The authors gratefully acknowledge the support of the Department of Otorhinolaryngology–Head and Neck Surgery at the Zagreb University Hospital Centre; the Merkur University Hospital, Zagreb; T-Com Croatia, Zagreb; InfoNET Projekt, Zagreb; and SiliconMaster, Zagreb.

### References

1. Klapan I, Simicic Lj, Pasarić K, et al. Realtime transfer of live video images in parallel with three-dimensional modeling of the surgical field in computer-assisted telesurgery. *J Telemed Telecare* 2002;8:125-30.
2. Klapan I, Simicic L, Risavi R, et al. Tele-3-dimensional computer-assisted functional endoscopic sinus surgery: New dimension in the surgery of the nose and paranasal sinuses. *Otolaryngol Head Neck Surg* 2002;127:549-57.
3. Mladina R, Hat J, Klapan I, Heinzel B. An endoscopic approach to metallic foreign bodies of the nose and paranasal sinuses. *Am J Otolaryngol* 1995;16:276-9.
4. Risavi R, Klapan I, Handzic-Cuk J, Barcan T. Our experience with FESS in children. *Int J Pediatr Otorhinolaryngol* 1998;43:271-5.
5. Hassfeld S, Muhling J. Navigation in maxillofacial and craniofacial surgery. *Comput Aided Surg* 1998;3:183-7.
6. Levine BA, Cleary KR, Norton GS, Mun SK. Experience implementing a DICOM 3.0 multivendor teleradiology network. *Telemed J* 1998;4:167-75.
7. Holtel MR, Burgess LP, Jones SB. Virtual reality and technologic solutions in otolaryngology [abstract]. *Otolaryngol Head Neck Surg* 1999;121:181.
8. Klapan I, Barbir A, Simicic L, et al. Dynamic 3D computer-assisted reconstruction of a metallic retrobulbar foreign body for diagnostic and surgical purposes. Case report of orbital injury with ethmoid bone involvement. *Orbit* 2001;20:35-49.
9. Klapan I, Simicic L, Besenski N, et al. Application of 3D computer-assisted techniques to sinonasal pathology—Case report: War wounds of paranasal sinuses caused by metallic foreign bodies. *Am J Otolaryngol* 2002;23:27-34.
10. Klimek L, Mosges R, Schlondorff G, Mann W. Development of computer-aided surgery for otorhinolaryngology. *Comput Aided Surg* 1998;3:194-201.
11. Mann W, Klimek L. Indications for computer-assisted surgery in otorhinolaryngology. *Comput Aided Surg* 1998;3:202-4.
12. Anon J. Computer-aided endoscopic sinus surgery. *Laryngoscope* 1998;108:949-61.